Oratect® Quick Reference Guide

1. **Remove** the cranberry color cap by holding the sides and pulling gently. This will expose the collection pad. **Make sure there is a blue line present in each window area indicating an unused device.**

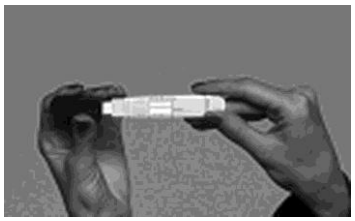

2. **Open** mouth and gently **rub** the collection pad inside mouth against cheek in a circular motion several (approximately 15-20) times. Make sure to **keep head level.**

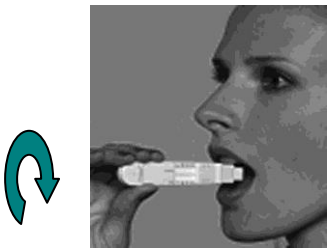

3. Gently **rub** the collection pad against the opposite cheek in circular motion several (approximately 15-20) times.

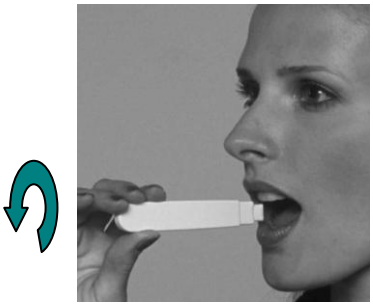

4. Gently **rub** the collection pad **on top** of the tongue several (approximately 15-20) times. **Do not chew, suck, bite or bend the collection pad.**

5. **Rub** the collection pad **underneath** the tongue several (approximately 15-20) times.

6. Place the collection pad underneath the tongue for approximately 30 seconds to collect saliva. Instruct the donor to hold the device in place with hand. **When sufficient amount of saliva is collected the blue lines will move. Repeat steps 2-6 until blue lines start to move upward**

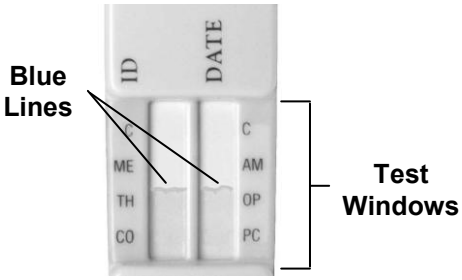

7. **Remove** from mouth as soon as blue lines move in both of the test windows. **Re-cap** the device.



8. Lay the device on a flat surface and **read results in approximately 5 minutes after removing the device from mouth. Read package insert.**

Interpreting Test Results

Invalid Result

When **no** colored band appears in the **CONTROL (C) region**, **the test is invalid** even if there is a band in the test region. **Repeat** the test with a new device.

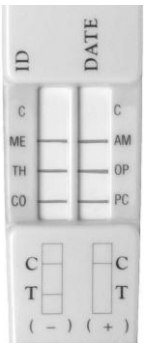

Example Interpretation:

ME: Invalid
TH: Invalid
CO: Invalid
AM: Invalid
OP: Invalid
PC: Invalid

Negative Result

For each test, two colored bands should be observed:

- **One in the CONTROL (C) region**
- **One in the specific TEST region**

The color of the test band may be slightly darker or lighter than the control band. Any visible band that can be seen is a **negative** result.

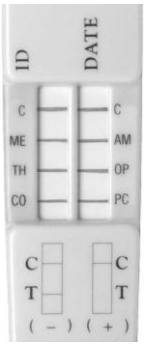

Example Interpretation:

ME: Negative
TH: Negative
CO: Negative
AM: Negative
OP: Negative
PC: Negative

Presumptive Positive Result

A colored band at the CONTROL (C) region should be observed. When there is no colored band or shadow band at the specific **TEST region**, the test is presumptive positive for that particular drug.

Example Interpretation:

ME: **Presumptive Positive**
TH: Negative
CO: Negative
AM: Negative
OP: Negative
PC: Negative